


# Test for Quaternary Sanitizer

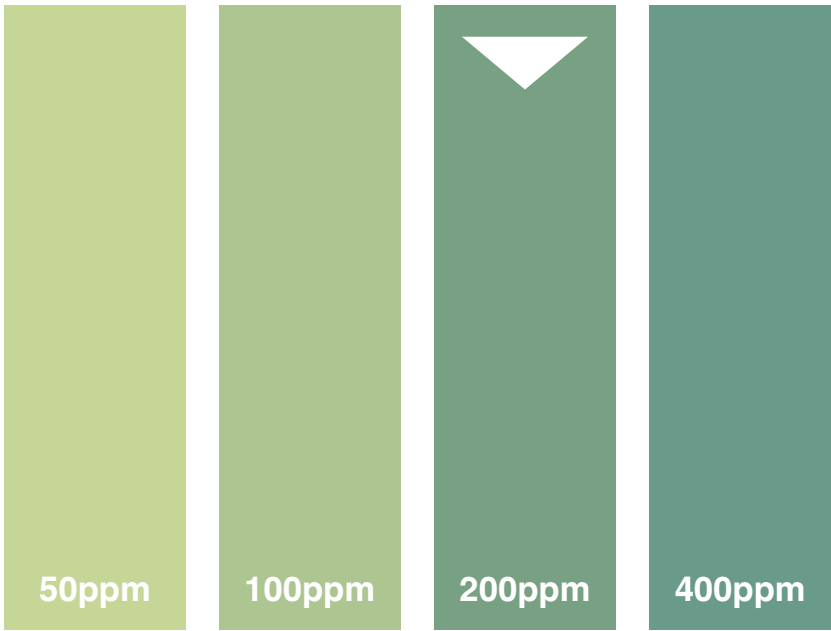

- Immerse pad in solution and remove immediately
- Hold strip level for 5 seconds
- Shake off excess water from pad
- Compare pad to the color chart

Keep out of sunlight

Keep vial closed when not in use

Sample must be above 75° F

Use dry fingers to remove test strip from vial



These instructions are for LaMatte item code 2951. Approximate color values are shown, accurate readings are to be made using the key provided with the test strips.